



Acoustic Imaging Camera

User Manual



Contact Us

Safety Instruction

These instructions are intended to ensure that user can use the product correctly to avoid danger or property loss.

Laws and Regulations

- Use of the product must be in strict compliance with the local electrical safety regulations.

Transportation

- Keep the device in original or similar packaging while transporting it.
- Keep all wrappers after unpacking them for future use. In case of any failure occurred, you need to return the device to the factory with the original wrapper. Transportation without the original wrapper may result in damage on the device and the company shall not take any responsibilities.
- DO NOT drop the product or subject it to physical shock. Keep the device away from magnetic interference.

Power Supply

- Please purchase the charger by yourself. Input voltage should meet the Limited Power Source (5 VDC, 2 A) according to the IEC61010-1 standard. Please refer to technical specifications for detailed information.
- Make sure the plug is properly connected to the power socket.
- DO NOT connect multiple devices to one power adapter, to avoid over-heating or fire hazards caused by overload.

Battery

- Improper use or replacement of the battery may result in explosion hazard. Replace with the same or equivalent type only. Dispose of used batteries in conformance with the instructions provided by the battery manufacturer.
- The built-in battery cannot be dismantled. Please contact the manufacture for repair if necessary.
- For long-term storage of the battery, make sure it is fully charged every three months to ensure the battery quality. Otherwise, damage may

occur.

- DO NOT charge other battery types with the supplied charger. Confirm there is no flammable material within 2 m of the charger during charging.
- DO NOT place the battery near heating or fire source. Avoid direct sunlight.
- DO NOT swallow the battery to avoid chemical burns.
- DO NOT place the battery in the reach of children.
- The lithium battery voltage is 3.6 V, and the battery capacity is 6230 mAh (22.43 Wh).

Maintenance

- DO NOT maintain the camera when it is powered on, or it may cause electric shock! If the product does not work properly, please contact your dealer or the nearest service center. We shall not assume any responsibility for problems caused by unauthorized repair or maintenance.
- Wipe the device gently with a clean cloth and a small quantity of ethanol, if necessary.
- If the equipment is used in a manner not specified by the manufacturer, the protection provided by the device may be impaired.
- Please notice that the current limit of USB 3.0 PowerShare port may vary with the PC brand, which is likely to result in incompatibility issue. Therefore, it's advised to use regular USB 3.0 or USB 2.0 port if the USB device fails to be recognized by PC via USB 3.0 PowerShare port.

Using Environment

- Make sure the running environment meets the requirement of the device. The operating temperature shall be -20 °C to 50 °C (-4 °F to 122 °F), and the operating humidity shall be 95% or less.
- Place the device in a dry and well-ventilated environment.
- DO NOT expose the device to high electromagnetic radiation or dusty environments.
- DO NOT aim the lens at the sun or any other bright light.
- When any laser equipment is in use, make sure that the device lens is not exposed to the laser beam, or it may burn out.
- The level of protection is IP 54. The device is suitable for indoor and outdoor uses, but do not expose it in wet conditions.

Technical Support

The <https://www.hikmicrotech.com/en/contact-us/> portal will help you access to our support team, software and documentation, service contacts, etc.

Emergency

If smoke, odor, or noise arises from the device, immediately turn off the power, unplug the power cable, and contact the service center.

Limited Warranty

Scan the QR code for the product warranty policy.






Manufacture Address

Room 313, Unit B, Building 2, 399 Danfeng Road, Xixing Subdistrict,
Binjiang District, Hangzhou, Zhejiang 310052, China

Hangzhou Microimage Software Co., Ltd

Symbol Conventions

The symbols that may be found in this document are defined as follows.

| Symbol | Description |
|---|---|
|  Danger | Indicates a hazardous situation which, if not avoided, will or could result in death or serious injury. |
|  Caution | Indicates a potentially hazardous situation which, if not avoided, could result in equipment damage, data loss, performance degradation, or unexpected results. |
|  Note | Provides additional information to emphasize or supplement important points of the main text. |

Contents

| | | |
|----------|--|-----------|
| 1 | Overview..... | 1 |
| 1.1 | Camera Description..... | 1 |
| 1.2 | Main Function..... | 1 |
| 1.3 | Appearance..... | 2 |
| 1.3.1 | Appearance: 64-Microphone Array..... | 2 |
| 1.3.2 | Appearance: 136-Microphone Array..... | 3 |
| 2 | Preparation | 6 |
| 2.1 | Mount Hand Strap | 6 |
| 2.2 | Operation Method..... | 7 |
| 2.3 | Charge Camera..... | 8 |
| 2.3.1 | Charge Camera via Cable Interface..... | 8 |
| 2.3.2 | Charge Camera via Charging Base | 9 |
| 2.4 | Power On/Off..... | 10 |
| 2.4.1 | Set Auto Power-off Countdown | 11 |
| 2.5 | Sleep and Wake | 11 |
| 2.6 | Auto Microphone Check | 12 |
| 2.7 | Live Interface and Menu | 12 |
| 2.7.1 | Live View Interface | 12 |
| 2.7.2 | Menus..... | 15 |
| 3 | Partial Discharge Detection (PD)..... | 17 |
| 3.1 | Partial Discharge Detection Operation..... | 17 |
| 3.2 | PD Types and Levels | 18 |
| 4 | Gas Leak Detection (LD)..... | 20 |
| 4.1 | Gas Leak Detection Operations..... | 21 |
| 4.1.1 | Estimated Cost Calculation for Compressed Air Leak | 22 |
| 4.1.2 | Estimated Cost Calculation for Bottled Gas Leak..... | 25 |
| 4.2 | Leak Rate Calibration | 26 |
| 5 | Basics of Acoustic Wave Detection | 27 |
| 5.1 | Set Frequency | 27 |
| 5.1.1 | Switch among Pre-defined Target Frequency Ranges | 27 |
| 5.1.2 | Set Target Frequency Range Manually..... | 28 |
| 5.2 | Set Industrial Frequency | 29 |
| 5.3 | Set Sound Source Distance | 30 |
| 5.3.1 | Set Manual Ranging..... | 30 |
| 5.3.2 | Set Auto Ranging | 30 |
| 5.4 | Set Detection Sensitivity | 31 |
| 5.5 | More Tools..... | 31 |

Acoustic Imaging Camera User Manual

| | | |
|-----------|---|-----------|
| 5.5.1 | Mark and Display Peak Intensity | 31 |
| 5.5.2 | Regional Detection Frame | 32 |
| 5.5.3 | Show Multiple Sound Sources | 32 |
| 5.5.4 | Ultrasonic to Audible | 33 |
| 6 | Display Settings | 35 |
| 6.1 | Set Acoustic Palettes | 35 |
| 6.1.1 | Set Palette Color | 35 |
| 6.1.2 | Set Palette Opacity | 35 |
| 6.1.3 | Set Intensity Range for Palettes | 36 |
| 6.2 | Adjust Digital Zoom | 36 |
| 6.3 | Set Grayscale of Visual Image | 37 |
| 6.4 | Set Video Standard | 37 |
| 6.5 | Set Screen Brightness | 37 |
| 6.6 | On-Screen Display Info. | 38 |
| 7 | Snapshot and Video | 39 |
| 7.1 | Capture Snapshot | 39 |
| 7.2 | Record Video | 40 |
| 7.3 | File Naming Rule | 41 |
| 7.4 | View and Manage Local Files | 41 |
| 7.4.1 | Manage Albums | 41 |
| 7.4.2 | Manage Files | 42 |
| 7.4.3 | Edit Files | 43 |
| 7.4.4 | Import and Manage Tag Note Templates | 44 |
| 7.5 | Export Files | 45 |
| 7.6 | Analyze Snapshot via HIKMICRO Analyzer Acoustic | 46 |
| 8 | Connections | 47 |
| 8.1 | Connect Camera to Wi-Fi | 47 |
| 8.2 | Set Camera Hotspot | 48 |
| 8.3 | Pair Bluetooth Devices | 49 |
| 8.4 | Connect to HIKMICRO Viewer APP | 49 |
| 9 | Cast Screen | 51 |
| 10 | Maintenance | 52 |
| 10.1 | View Camera Information | 52 |
| 10.2 | Set Language | 52 |
| 10.3 | Set Time and Date | 52 |
| 10.4 | Upgrade Camera | 52 |
| 10.4.1 | Upgrade with HIKMICRO Viewer APP | 52 |
| 10.4.2 | Upgrade with an Upgrade File | 53 |
| 10.5 | Restore Camera | 53 |
| 10.6 | Record Sound Source for Trouble Shooting | 54 |
| 10.7 | Save Log | 54 |
| 11 | More Information | 56 |

1 Overview

1.1 Camera Description

The HIKMIRCO acoustic imaging camera is a professional product for sound source positioning. With its low-noise MEMS microphones and adjustable bandwidth range, it provides an easy and effective way to locate the pressurized gas leaks or partial discharge in industrial environments. By using a large 4.3" LCD touch screen, the results overlaying on a visual image allows you to quickly find the source of the problems. Adopting this lightweight and easy-to-use tool, you can discover the potential safety risks, minimize troubleshooting, and save extra costs of equipment failures and downtime.

1.2 Main Function

Acoustic Imaging

Camera detects the real-time sound intensity of the sources, and locates the sources in the scene.

Partial Discharge Detection (PD)

Camera detects partial discharge activities and estimates their types based on sound frequency, and displays the real-time estimation in live view for your reference.

Gas Leak Detection (LD)

Camera detects and estimates real-time gas leak rate, leak cost, and leak level for reference.

Palettes

Camera supports multiple palettes to display the detected sound sources and their intensities.

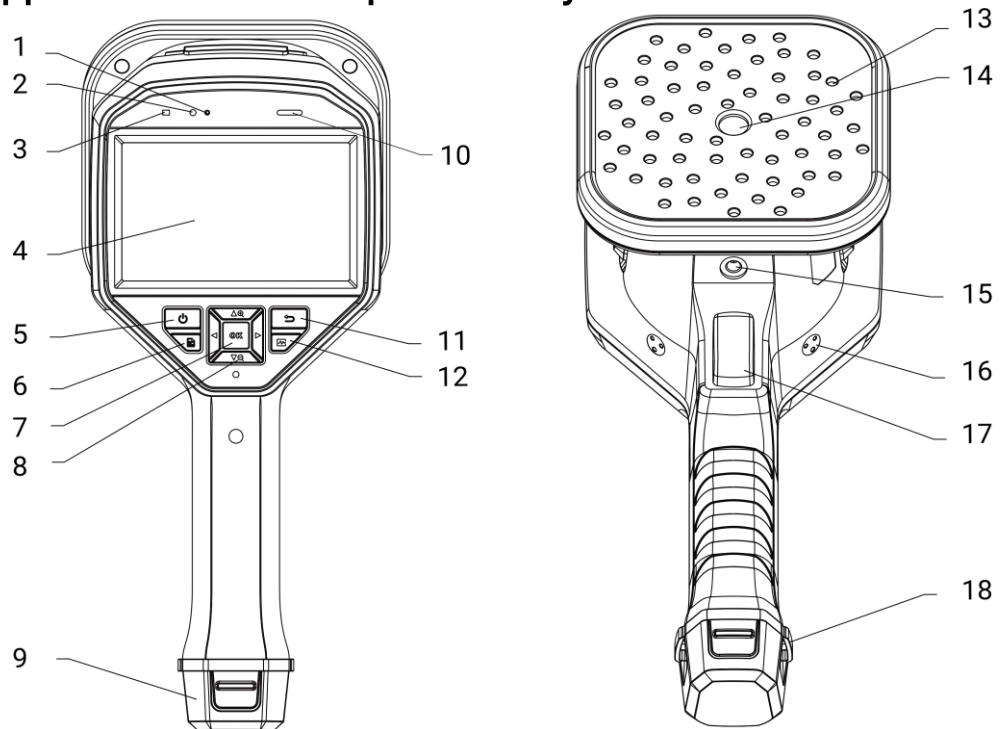
Record Videos & Capture Snapshots

Camera supports recording videos, capturing snapshots, and managing albums.

1.3 Appearance

There are two types of the acoustic imaging camera in this series with different microphone array (No.13 in the following figures).

1.3.1 Appearance: 64-Microphone Array



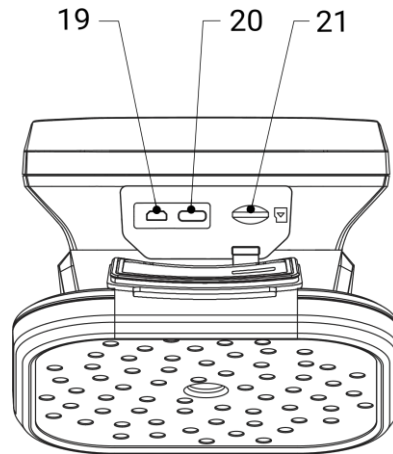


Figure 1-1 Appearance: 64-Microphone Array

1.3.2

Appearance: 136-Microphone Array

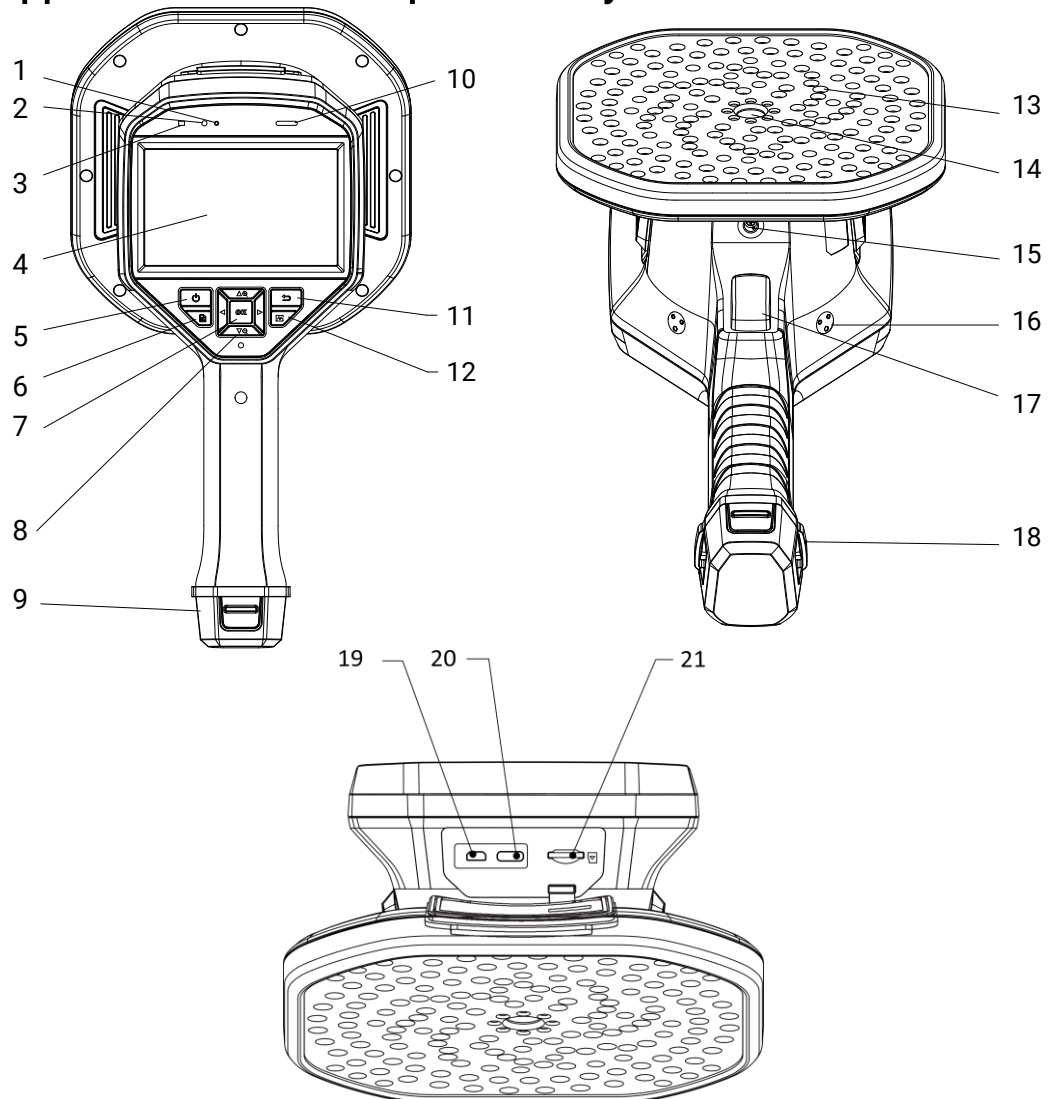
















Figure 1-2 Appearance: 136-Microphone Array

Table 1-1 Interface Description

| No. | Component | Function |
|-----|------------------------------|---|
| 1 | Light Sensor | Senses the ambient brightness. |
| 2 | Microphone | Records voice notes. |
| 3 | Power Indicator | Solid red: Charge normally. Solid green: Fully charged. |
| 4 | LCD Touch Screen | Allows live view and touch-screen operation. |
| 5 | Power Button | Holds  to power on/off. Presses  to enter/exit sleep mode. |
| 6 | File Button | Presses  to access the albums. |
| 7 | Confirm Button | Non-Menu Mode: Press  to enter menu. Menu Mode: Press  to confirm. |
| 8 | Navigation Button | Non-Menu Mode: <ul style="list-style-type: none"> ● Presses  or  to zoom in or zoom out by 0.1× continuously. ● Holds  or  to zoom in or zoom out by 1× continuously. Menu Mode: Presses  ,  ,  , and  to select parameters. |
| 9 | Battery Compartment | For holding the battery. |
| 10 | Loudspeaker | Plays voice notes. |
| 11 | Back Button | Presses  to save the parameters and returns to previous menu. |
| 12 | Frequency Button | Presses to select the frequency range frame edges and configures the frequency parameters. |
| 13 | Microphone Array | Detects sound in the scene. |
| 14 | Visual Camera | Views the visual images. |
| 15 | Tripod Attachment Point | Mounts the tripod. |
| 16 | Hand Strap Attachment Points | Mounts the hand strap. |
| 17 | Trigger | Non-Menu Mode: <ul style="list-style-type: none"> ● Presses: Capture snapshots. ● Holds: Record videos. Menu Mode: Presses to return to live view interface. |

| | | |
|----|-----------------------------|--|
| 18 | Hand Strap Attachment Holes | Fixes the lower part of the hand strap to the camera. |
| 19 | Micro HDMI Interface | Displays the image and menu interface via HDMI output. |
| 20 | Type-C Interface | Charges the camera or exports files with supplied cable. |
| 21 | MicroSD Card Slot | For holding the MicroSD card. |

2 Preparation

2.1 Mount Hand Strap

The hand straps aim at attaching to the camera and stabilizing it. Please make sure that your hands are wrapped with the hand straps to prevent the camera from accidental falling or bumping.

The upper part of the hand strap is attached to the camera by a buckle. There are two buckle attachment points on both sides of the camera. The lower part of the hand strap is threaded through the holes at the base of the camera.

1. Insert the upper part of the hand straps into the buckles.

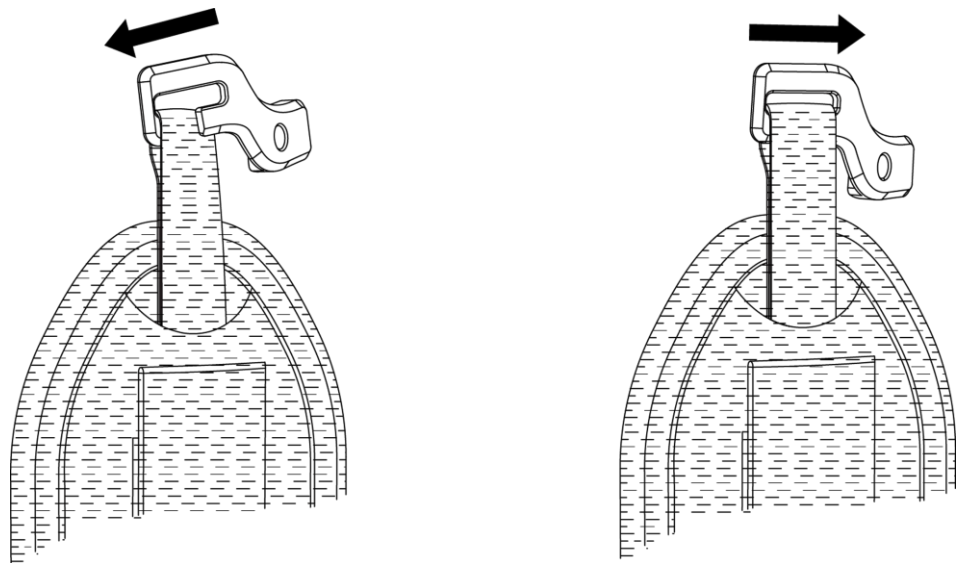


Figure 2-1 Insert Upper Part of Hand Strap

2. Fit the buckle on the camera and tighten the screw with the supplied wrench.
3. Thread the lower part of the hand strap through the hole at the base of the camera.

4. Secure the hand strap with the hook-and-loop fastener. Adjust the tightness according to your hands.

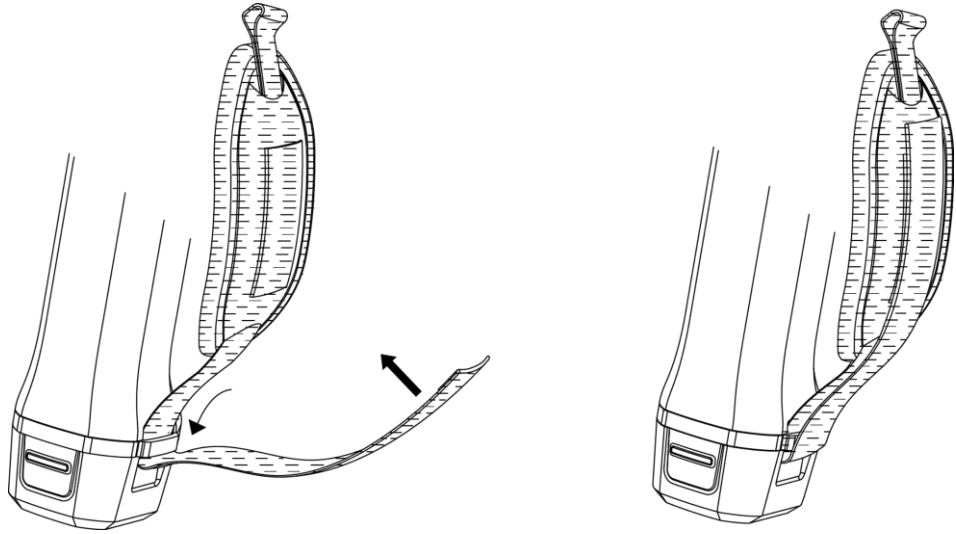


Figure 2-2 Secure Lower Part of Hand Strap

2.2 Operation Method

The camera supports both touch-screen control and button control.

Touch-Screen Control

Tap on the screen to set parameters and configurations.

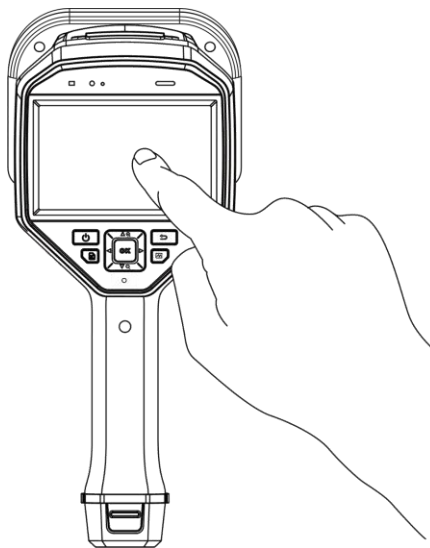


Figure 2-3 Touch-Screen Control

Button Control

Press the navigation buttons to set parameters and configurations.

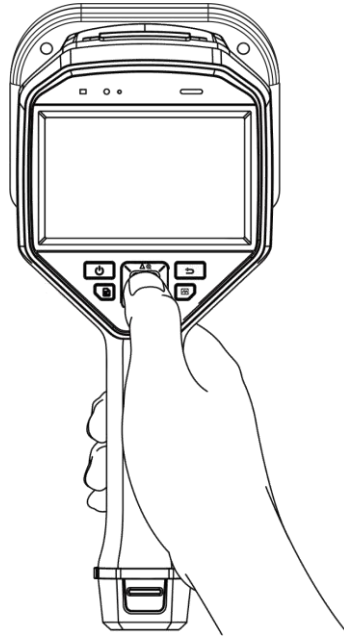


Figure 2-4 Button Control

2.3 Charge Camera

Please fully charge the camera before it is used for the first time or when it is in low battery.

2.3.1 Charge Camera via Cable Interface

Before You Start

Please make sure the battery is installed before charging via cables.

Steps

1. Open the connector cover of the camera.
2. Plug the Type-C male connector of the charging cable to the camera and the other type-A connector to power adapter.

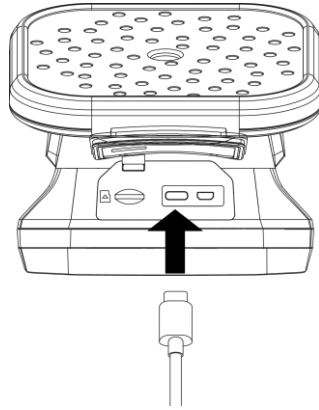


Figure 2-5 Charge via Type-C Cable



For device with 64-Microphone Array, the power delivered by the charger must be between min 9 Watts required by the radio equipment, and max 10 Watts in order to achieve the maximum charging speed.

For device with 136-Microphone Array, the power delivered by the charger must be between min 9 Watts required by the radio equipment, and max 15 Watts in order to achieve the maximum charging speed.

2.3.2 Charge Camera via Charging Base

You can take out the battery and insert it into the charging base for fast charging.

Before You Start

Please make sure the camera is power off before removing the battery.

Steps

1. Hold the camera, and press both battery lock catches of the camera.

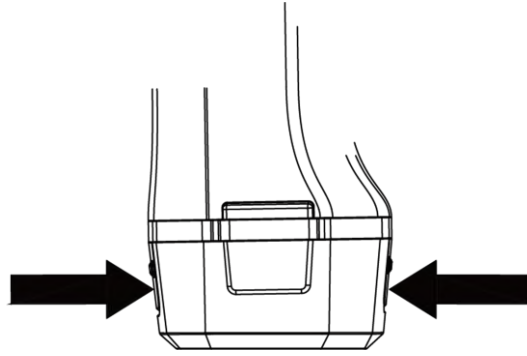


Figure 2-6 Remove Battery Base

2. Hold the lock catches, and draw the battery base to take out the battery.
3. Insert the battery into the charging base. You can see the charging status via the pilot lamp on the charging base.



The red indicating light is on if the battery is charging properly, and the green indicating light is on if the battery is fully charged.

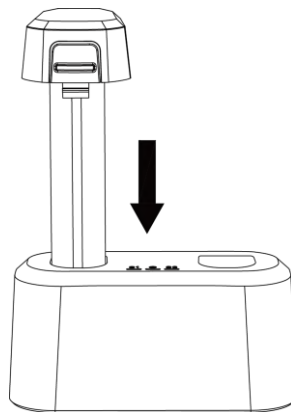



Figure 2-7 Charge Battery

4. When the battery is fully charged, draw the battery from the charging base.
5. Insert the battery into the camera and push it into the locked position.

2.4 Power On/Off


Power On

Hold  to turn on the camera. You can observe the target when the live view interface is stable.






If the battery of the camera is low, please charge it in time or replace it with a fully-charged standard battery, so as to ensure that the camera functions normally.

Power Off

When the camera is turned on, hold  to power off the camera.

2.4.1 Set Auto Power-off Countdown

Steps

1. Press  in live view interface to show the menu.
2. Go to **Settings > Device Settings > Auto Power-off**.
3. Select **Auto Power-off** and press  to enable auto power-off.
4. Set the automatic shutdown time for camera as required.
5. Press  to save and return to previous menu.


2.5 Sleep and Wake

Sleep and wake is used to save energy and increase battery time.

Sleep and Wake Manually


Press  to enter sleep mode and press again to wake camera up.

Set Auto Sleep

In live view, press  to call the main menu. Go to **Settings > Device Settings > Auto Sleep** to set waiting time before auto sleep.

When there is no button pressing or screen tapping operation on camera for more than the set waiting time, camera enters sleep mode automatically.

Camera Sleep, Scheduled Capture and Video Recording

When the camera is recording a video clip or on scheduled capturing, auto sleep will not be triggered. However, press  will stop the video recording or scheduled capture and force the camera into sleep mode.

2.6 Auto Microphone Check

Auto microphone check is a camera self-test on the microphone array.

Go to **Settings > Device Settings > Auto Microphone Check** for the test. If microphone error is detected, please contact your dealer or our technical support for help.

2.7 Live Interface and Menu

2.7.1 Live View Interface

After starting up, camera screen shows the live view interface with detected acoustic wave.

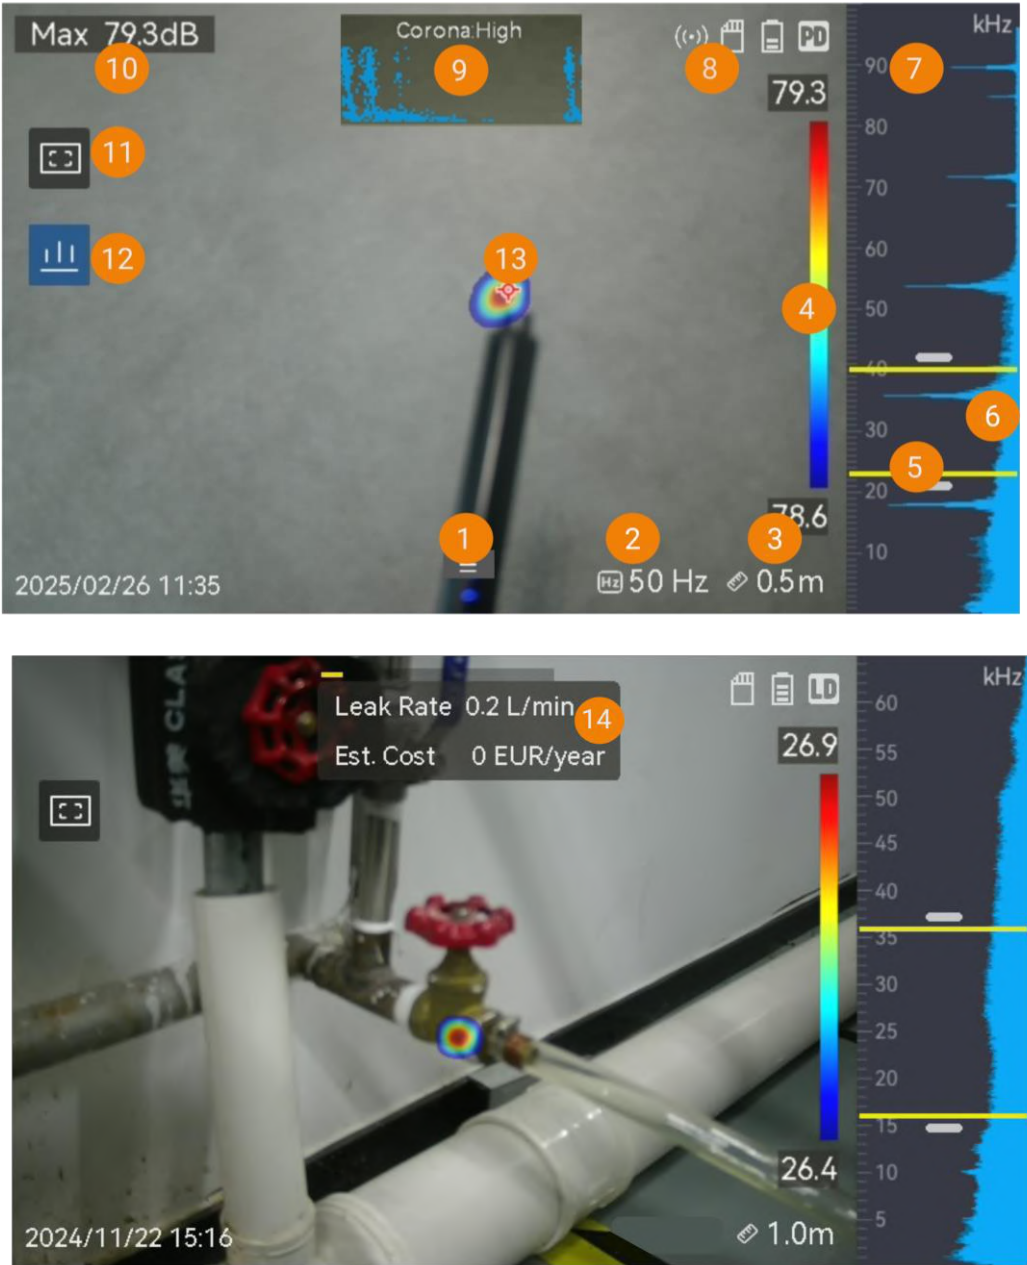


Figure 2-8 Live View Interface



Table 2-1 Live View Interface Description

| No. | Part Name | Function |
|-----|-----------------------|--|
| 1 | Menu Icon | Taps on the icon to call the main menu. |
| 2 | Industrial Frequency | Sets the industrial frequency of the target. See 5.2 Set Industrial Frequency. |
| 3 | Sound Source Distance | Shows the set distance of sound source. See 5.3 Set Sound Source Distance. |

| No. | Part Name | Function |
|--------|--------------------------------------|--|
| 4 | Intensity Scale (Palette Bar) | Intensity scale (palette bar) shows the relation between displayed color and sound intensity. The value at the ends of the bar stands for the maximum and minimum intensity of the set frequency range. See <i>6.1.1 Set Palette Color</i> for setting instructions. |
| 5 | Selected (Target) Frequency Range | Sound intensity of this frequency band is detected and converted to acoustic palette. See <i>5.1 Set Frequency</i> for instructions. |
| 6 | Dynamic Intensity of All Frequencies | Shows the intensity change of supported frequencies. |
| 7 | Frequency Band | Shows the supported frequency band of the camera. |
| 8 | Status Bar | Displays the camera working status at the top right. Turn on/off the display from Settings > Display Settings > Status Icons . |
| 9 & 12 | PRPD and its Control Icon | Only available in PD mode. Taps on icon (12) to display phase resolved partial discharge (PRPD) diagram for better PD activity diagnosis. Taps on PRPD diagram (9) to enlarge the display. |
| 10 | Maximum Intensity | Stands for the detected maximum intensity of the scene. See <i>5.5.1 Mark and Display Peak Intensity</i> for setting instructions. |
| 11 | Regional Detection Frame | Taps on the icon to show a frame in the middle of the screen. The camera only displays sound sources in the frame to reduce interference from less interested areas. See <i>5.5.2 Regional Detection Frame</i> for more information. |

| No. | Part Name | Function |
|-----|------------------|--|
| 13 | Acoustic Palette | The location and intensity of detected sound source are converted to palette colors overlaying on the visual image for easy observation. The size of palette stands for the intensity of the sound source. Bigger acoustic palette covered area means wider sound intensity range. |
| 14 | Gas Leak Info. | Only available in LD mode. Shows detected gas leak estimation. See <i>4 Gas Leak Detection (LD)</i> for more information. |

2.7.2 Menus

In live view interface, tap  or press  to show the main menu, and swipe down to call the swipe-down menu.

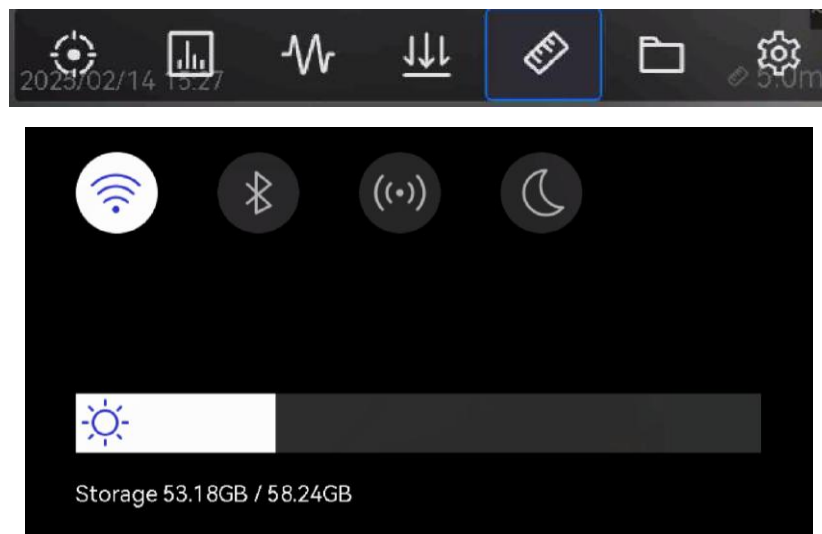














Figure 2-9 Main Menu and Swipe-Down Menu

Table 2-2 Menu Description

| Menu Icon | Function |
|---|--|
|  | Detection mode switch. Partial Discharge Detection (PD) and Gas Leak Detection (LD) are supported. |
|  | Adjusts detection sensitivity. Higher level means higher sensitivity. See <i>5.4 Set Detection Sensitivity</i> for setting instructions. |




| Menu Icon | Function |
|---|---|
|  | Pre-defined target frequency ranges for quick switching. |
|  | Adjusts system pressure of the target in LD mode only. See <i>4.1 Gas Leak Detection Operations</i> for setting instructions. |
|  | Distance to sound source. |
|  | Local albums of captured images and videos. See <i>7.4 View and Manage Local Files</i> for setting instructions. |
|  | Settings of all camera functions. |
|  | Taps to turn on/off camera Wi-Fi. See <i>8.1 Connect Camera to Wi-Fi</i> for setting instructions. |
|  | Taps to turn on/off camera Bluetooth. See <i>8.3 Pair Bluetooth</i> for setting instructions. |
|  | Taps to turn on/off camera hotspot. See <i>8.2 Set Camera Hotspot</i> for setting instructions. |
|  | Taps to switch menu themes between dark and light. |
|  | Swipes to adjust screen brightness. |

3 Partial Discharge Detection (PD)

Partial discharge detection is often used in electrical equipment and facility inspection. It detects abnormal partial discharges faults and instructs maintenance activities.

3.1 Partial Discharge Detection Operation

Steps

1. In live view interface, tap  or press  to show the menu.
2. Select  to switch detection mode to PD.
3. Set industrial frequency of the target. Industrial Frequency refers to the working electrical frequency of the observed targets. It affects the accuracy of acoustic detection. See *5.2 Set Industrial Frequency*.
4. Set detection distance. Measure the distance between the microphone array to the target and input the data to the camera. See *5.3 Set Sound Source Distance*.
5. Hold and aim the microphone array to the target.
6. (Optional) If the target sound source intensity is weak and there is much interference around, enable the regional detection frame. See *5.5.2 Regional Detection Frame*.
7. (Optional) If you want to listen to the detected ultrasonic sound source (usually inaudible to human ears) for double confirm, enable **Ultrasonic to Audible** and connect your camera to a pair of Bluetooth headsets. See *5.5.4 Ultrasonic to Audible* and *8.3 Pair Bluetooth*.
8. Adjust the selected frequency range. See *5.1 Set Frequency*.
9. Adjust detection sensitivity. See *5.4 Set Detection Sensitivity*.
10. Check acoustic palettes position, maximum sound intensity position, PRPD diagram and the detection result on screen. To read the result, see *3.2 PD Types and Levels*.

11. Take snapshots or record videos of the suspected sound sources. See *7 Snapshot and Video*.

3.2 PD Types and Levels

When detecting a partial discharge sound source, camera automatically identifies the type and strength level, and displays the result on screen.



Due to potential environmental factors that may affect detection accuracy, PD type and strength level provided are approximate and for informational purposes only.

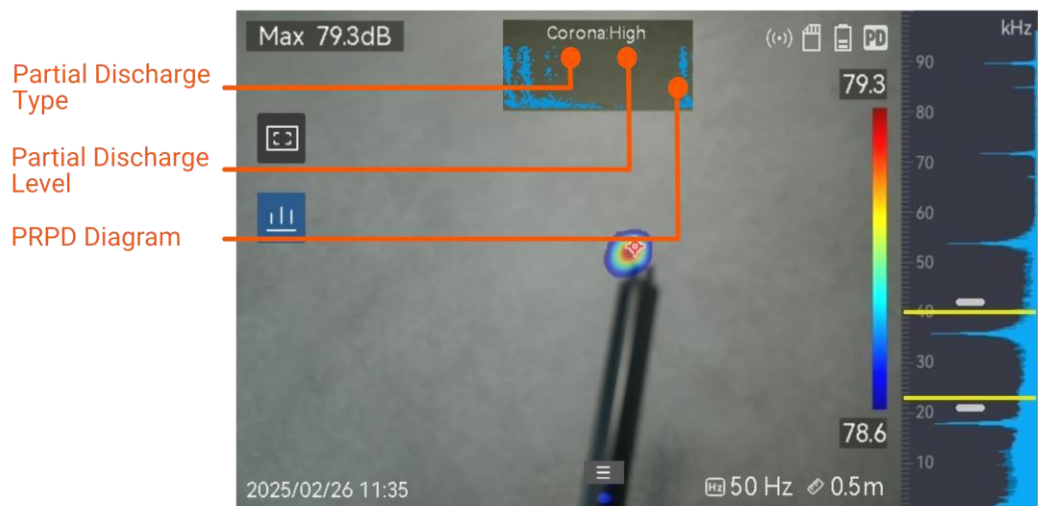


Figure 3-1 Partial Discharge Display

The explanation of screen display and the recommended handling are shown in the following tables.

Table 3-1 Partial Discharge Types

| Partial Discharge Types | Description |
|-------------------------|--|
| Corona | Corona discharge occurs on the sharp surface of a conductor surrounded by gas. It usually happens in electrical systems like high-voltage power lines, transformers, or electrical motors. |

| Partial Discharge Types | Description |
|-------------------------|--|
| Floating | Floating discharge, one of arcing discharges, happens when the electrical current flows through the conducting path created by voltage difference between two conductors. It might occur in various situations, such as high-voltage power transmission systems, electrical switches, circuit breakers, and welding equipment. |
| Surface | Surface discharge refers to the electrical discharge travels along the surface of insulation. It is primarily caused by the contamination and weather conditions like high humidity, of the insulator surface. It often occurs in high-voltage equipment, such as transformers, cables, switchgear, and motors. |
| Particle | Particle discharge refers to the partial discharge of electrical energy that interacts with metallic particles and debris present in the electrical systems. It can result from loose particles or particles generated by mechanical wear, corrosion, or degradation of insulation materials. |
| Noise | Other detected sound. |

If different types of partial discharges coexist in the scene, the most prominent partial discharge type shows in live view.

Table 3-2 Partial Discharge Severity and Handling

| Partial Discharge Severity | Recommended Handling |
|----------------------------|--|
| Normal | No observable/measurable deterioration. |
| Low | Minor deterioration which requires attention. Shorten inspection period and take maintenance actions when necessary. |
| Medium | Moderate deterioration. Locate and clean the Item during routine maintenance, or carry out related electrical test of the item. Or use online monitor to monitor the discharge tendency. |
| High | Serious deterioration. Item can not be returned to service without shutdown or engineering advise. |

4 Gas Leak Detection (LD)

LD mode is often used in gas leak detection of gas pipelines, tanks, valves, etc.

In LD, there are 2 gas leak modes with different calculations of leak cost. Select a leak mode according to the inspected target and the way of cost calculation.

Table 4-1 Gas Leak Modes

| Gas Leak Mode | Description |
|----------------|--|
| Bottled Gas | Locate leak points and detect leak rate. Calculate estimated cost according to the price of gas and leak rate. See <i>4.1.2 Estimated Cost Calculation for Bottled Gas Leak</i> for leak cost calculation. |
| Compressed Air | Locate leak points and detect leak rate. The leak cost is the cost of extra power that the air compressor consumed to maintain system pressure. The power waste can also be converted to CO2 emissions for display. See <i>4.1.1 Estimated Cost Calculation for Compressed Air Leak</i> for leak cost calculation. |









This product is designed to assess gas leak to achieve cost savings. However, due to potential environmental factors that may affect detection accuracy, the estimations provided are approximate and for informational purposes only. It should be noted that the results presented by the camera are not a guarantee of actual cost savings or a recommendation, and may not accurately reflect the specific situation of your facilities.

4.1 Gas Leak Detection Operations








The following procedure is a general operation guide. Fine-tune the detection by adjusting frequency, distance, and sensitivity to find solid and stable leak points.



Steps

1. In live view interface, tap  or press  to show the menu.
 2. Select  to switch detection mode to LD.
 3. Go to **Settings > Acoustic Settings > Gas Leak Settings > Gas Leak Mode**, and set the mode as **Bottled Gas** or **Compressed Air**. See *Table 4-1* for mode difference.
 4. (Optional) Set the pressure for the target, generally container or pipes. The parameter helps improve accuracy when detecting small leaks.
 - 1) Tap on  in the main menu.
 - 2) Adjust the value with left/right navigation buttons, or tap on  .
-



Pressure unit can be changed from **Settings > Acoustic Settings > Gas Leak Settings > Unit Settings > Pressure**.

5. Set the parameters for result display and cost calculation.
 - For cost calculation of compressed air leak, see *4.1.1 Estimated Cost Calculation for Compressed Air Leak* for details.
 - For cost calculation of bottled gas leak, see *4.1.2 Estimated Cost Calculation for Bottled Gas Leak* for details.
 6. Set leak level. Manually adjust the range of each level.
 - 1) Select , and go to **Acoustic Settings > Gas Leak Settings > Leak Level**.
 - 2) Press  button, and choose a range in Leak Level interface.
 - 3) Press  button, and input the value in the box with a soft keyboard on screen.
 - 4) Tap  or press  button to confirm the settings.
-

7. Set detection distance. Measure the distance between the microphone array to the target and input the data to the camera. See *5.3 Set Sound Source Distance*.
8. Hold and aim the microphone array to the target.
9. (Optional) If the target sound source is small and there is much interference around, enable the regional detection frame. See *5.5.2 Regional Detection Frame*.
10. (Optional) If you want to listen to the detected ultrasonic sound source (usually inaudible to human ears) for double confirm, enable Ultrasonic to Audible and connect your camera to a pair of Bluetooth headsets. See *5.5.4 Ultrasonic to Audible* and *8.3 Pair Bluetooth*.
11. Adjust the selected frequency range. See *5.1 Set Frequency*.
12. Adjust detection sensitivity. See *5.4 Set Detection Sensitivity*.
13. (Optional) Enable **Stabilization** to stabilize the value of **Leak Rate** at the center of live view interface.
 - 1) Select , and go to Acoustic Settings > Gas Leak Settings > Stabilization.
 - 2) Press  button to turn on the function.
14. Check acoustic palettes position, maximum sound intensity position, and the detection result on screen.

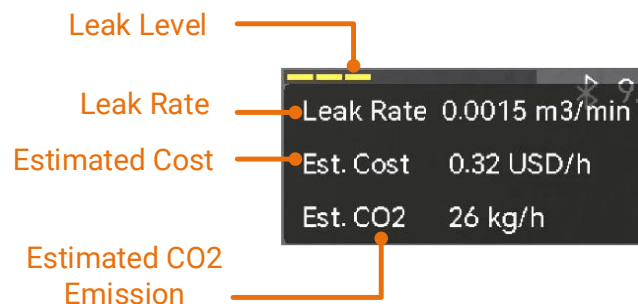


Figure 4-2 Gas Leak Estimation (Compressed Air)

15. (Optional) Calibrate the leak rate if you find it is deviated from the actual amount. See *4.2 Leak Rate Calibration*.
16. Take snapshots or record videos for the suspected sound sources. See *7 Snapshot and Video*.

4.1.1 Estimated Cost Calculation for Compressed Air Leak

There are 3 formulas involving different air compressor parameters for you to calculate leak cost and CO2 emission. Select a formula in which the required air compressor parameters are easy to obtain.

The estimated cost and CO2 emission are displayed at the top center of live view.

Steps




1. Switch gas leak mode to **Compressed Air** by  > **Acoustic Settings** > **Gas Leak Settings** > **Gas Leak Mode**.
2. Set **Currency**, **Leak Rate Unit**, **Leak Cost Time Unit** and **Pressure** unit for your calculation by  > **Acoustic Settings** > **Gas Leak Settings** > **Unit Settings**.
3. Select a formula according to the required air compressor parameters already known or easily accessed, and input corresponding values for calculation.
 - 1) Select a formula. Select , and go to **Acoustic Settings** > **Gas Leak Settings** > **Compressed Air Settings** > **Formula**.

Table 4-2 Recommended Formula for Compressed Air Leak

| Already Known/Available Parameters | Recommended Formula |
|--|---|
| Air Compressor Specific Power (Y) | Formula One: Est. CO2= $T \cdot X \cdot Y \cdot B$ Est. Cost= $T \cdot X \cdot Y \cdot A$ |
| <ul style="list-style-type: none">● Air Compressor Out Flow Rate (Q)● Air Compressor Power Consumption (P) | Formula Two: Est. CO2= $T \cdot X \cdot P \cdot B / Q$ Est. Cost= $T \cdot X \cdot P \cdot A / Q$ |
| <ul style="list-style-type: none">● Air Compressor Output Pressure (p)● Air Compressor Motor Efficiency (η) | Formula Three: Est. CO2= $T \cdot (p \cdot X \cdot B) / (\eta \cdot 60)$ Est. Cost= $T \cdot (p \cdot X \cdot A) / (\eta \cdot 60)$ |



Table 4-3 Parameters Description in Cost Calculation Formula





| Formula | Parameter | Description |
|---------|-----------|---|
| All | T | Working hours of the air compressor per day/month/year. Its unit depends on Leak |


| Formula | Parameter | Description |
|---------------------------|-----------|---|
| formulas | | Cost Time Unit. |
| | X | Leak rate of the target. It is an automatic measured value. The unit depends on Leak Rate Unit . |
| | A | The price of 1 kWh electricity. Its unit depends on Currency . |
| | B | CO2 emissions per kWh (carbon emissions from electricity). It can be obtained by querying the carbon emission factor of the local power grid. |
| Formula one only | Y | Air compressor specific power, indicating the working efficiency of an air compressor, is the ratio of input power to compressed air flow rate at a given pressure. It can be found in the data sheet of the air compressor. |
| Formula two only | P | Air compressor power consumption (Unit: kW). |
| | Q | Air compressor out flow rate, indicating gas quantity output by air compressor. |
| Formula three only | p | Air compressor output pressure, indicating generated pressure of the compressed air ventilated through air compressor. |
| | η | Air compressor motor efficiency (Unit: %). |



- The units of **Air Compressor Specific Power (Y)** and **Air Compressor Out Flow Rate (Q)** depend on **Leak Rate Unit**.
 - The unit of **Air Compressor Output Pressure (p)** is consistent with **Pressure**.
-

- Tap  at the right side of the formula to get specific meaning of each parameter. Press  or tap **Off** to hide the pop-up window.
-

- 2) Input corresponding parameter values.
 - Press  to return to **Compressed Air Settings** interface.
 - Select a parameter, and press  to enter the setting interface.
 - Input the value with the soft keyboard.
 - Press  or tap  to confirm the settings.

4. Press  to return to live view interface, and browse gas leak information at the screen center.
-





Due to potential environmental factors that may affect detection accuracy, the estimations provided are approximate and for informational purposes only.

4.1.2

Estimated Cost Calculation for Bottled Gas Leak






The cost of bottled gas leak is equal to the leak rate multiplied by price of the gas.

Steps

1. Switch gas leak mode to **Bottled Gas** by  > **Acoustic Settings** > **Gas Leak Settings** > **Gas Leak Mode**.
 2. Set leak rate unit and currency unit by  > **Acoustic Settings** > **Gas Leak Settings** > **Unit Settings**.
-



The unit of **Price of Gas** depends on **Leak Rate Unit** and **Currency**. For example, if users choose “L/min” as gas flow unit and “USD” as currency, the unit of gas price is “USD/L”.

3. Input the value of **Price of Gas**.
 - 1) Select , and go to **Acoustic Settings** > **Gas Leak Settings** > **Bottled Gas Settings** > **Price of Gas**.
 - 2) Press  to enter the setting interface.
 - 3) Input the value with the soft keyboard on screen.
 - 4) Press  or tap  to confirm the settings.
 4. Press  to return to live view interface.
-



Due to potential environmental factors that may affect detection accuracy, the estimations provided are approximate and for informational purposes only.





4.2 Leak Rate Calibration

If you find the leak rate is deviated from the actual amount, set a calibration factor for each leak rate range.

Calibrated leak rate = the detected leak rate × the set calibration factor.

You can set different calibration factors for different leak rate ranges. Calibration factor is a number from 0.000000 to 10.000000, up to 6 decimal places allowed.

Steps

1. In live view interface, tap  or press  to show the menu.
2. Select  to switch detection mode to LD.
3. Go to **Settings > Acoustic Settings > Gas Leak Settings > Leak Rate Calibration**.
4. Press  to enable the function.
5. Select a range to calibrate, and input a factor number by the soft keyboard for the range.



Leak rate ranges are camera provided, and set a calibration factor for each range in use.

6. Press  to confirm the settings and set factors for other ranges.

5 Basics of Acoustic Wave Detection

The camera supports acoustic wave detection among different frequency ranges. Detected sound source is marked with shaped acoustic palettes to show its dynamic location and intensity.

5.1 Set Frequency

Steps

1. The camera supports sound detection of two configurable frequency bands with different upper limit. Choose the one that better covers possible target frequencies from **Settings > Acoustic Settings > Frequency Band**.
2. Select a target frequency band, and sound of which is visualized to acoustic palettes in the display for easy observation. You can switch among pre-defined frequency ranges or adjust manually.

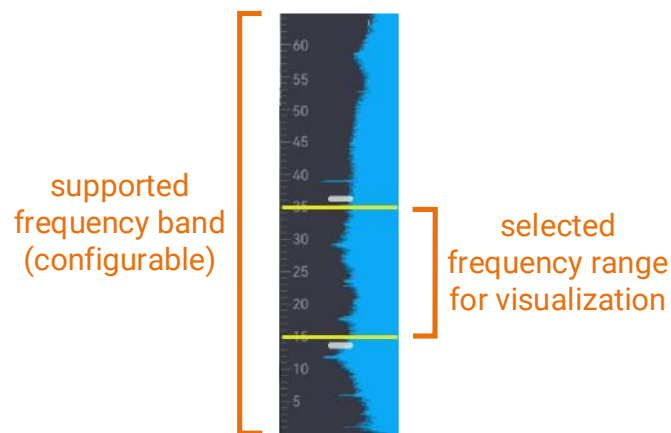


Figure 5-1 Frequency







Frequency modes are different in PD mode and LD mode.

5.1.1 Switch among Pre-defined Target Frequency Ranges

Switch Auto Frequency

Steps





1. Tap  or press  in live view to show the main menu.
2. Select .
3. Press  to switch to auto frequency, including low, middle and high levels.



Manual adjustment to the selected frequency band is not allowed in this mode.

Customize the frequency range

Steps






1. Tap  or press  in live view to show the main menu.
2. Customize the frequency band and set it as a predefined one.
 - 1) Select .
 - 2) Press  to start editing.
 - 3) Adjust the value of the selected frequency band on the right side.
See 5.1.2 Set Target Frequency Range Manually.



ONLY PD mode supports  custom frequency band.

5.1.2 Set Target Frequency Range Manually

Steps

1. Tap  or press  in live view to show the main menu
2. Select .
3. Press  and switch to .



ONLY PD mode supports  Manual Frequency.









4. Press  to save and exit.
5. Select a subject for adjustment.

Table 5-1 Selected Frequency Adjustment

| Objective | Operation | Operation Result |
|---|---|--|
| Adjust the upper and lower limits together. | Press  once or tap the area between the lines. |  |
| Adjust the upper limit only. | Press  twice or tap on the upper line. |  |
| Adjust the lower limit only. | Press  three times or tap on the lower line. |  |

6. Press/hold navigation buttons to adjust values.
7. Press  to save and exit.

5.2 Set Industrial Frequency

Due to different working frequency of the target, generally the electrical equipment, users can adjust industrial frequency to improve inspection accuracy.



- ONLY PD mode supports industrial frequency function.
- If **Video Standard** is switched, the value of industrial frequency is changed simultaneously. The default values of industrial frequency in PAL and NTSC are 50 Hz and 60 Hz respectively. See *6.4 Set Video Standard* for instructions.

Steps

1. Tap  > **Acoustic Settings** > **Industrial Frequency**.

2. Press  or  to save and exit.

5.3 Set Sound Source Distance














Distance to sound source helps to increase the acoustic wave detection accuracy.



ONLY LD mode supports Auto Ranging.






5.3.1 Set Manual Ranging

Steps


1. In live view, tap  or press  to show the menu.
2. Select .
3. Adjust the distance value.
 - PD mode: Press/hold  and , or tap  and .
 - LD mode: Choose , and then press/hold  and  or tap  and .
4. Press  to save and exit.

5.3.2 Set Auto Ranging

Steps

1. Turn off multiple sources mode from  > **Acoustic Settings** > **Multiple Sources**.
2. In live view, tap  or press  to show the menu.
3. Switch to LD mode.
4. Select  > , and the device automatically calculate the source distance.









- If there is no acoustic palette, “~” is displayed on the bottom right in live view.
 - Set distance unit from  > **Device Settings** > **Unit** > **Distance**.
-

5.4 Set Detection Sensitivity

Higher sensitivity means that sound source of lower intensity can be detected. Higher sensitivity also means that interferences are more easily to be detected and displayed.

Steps

1. In live view interface, tap  or press  to show the menu.
2. Select .
3. Press  and  or tapping on screen to select a level. Higher level means better sensitivity.
4. Press  to save and exit.

5.5 More Tools

5.5.1 Mark and Display Peak Intensity


Mark peak intensity point with  and display the peak intensity value on screen.



Figure 5-2 Mark Peak Intensity


Steps

1. In live view interface, tap  or press  to show the menu.

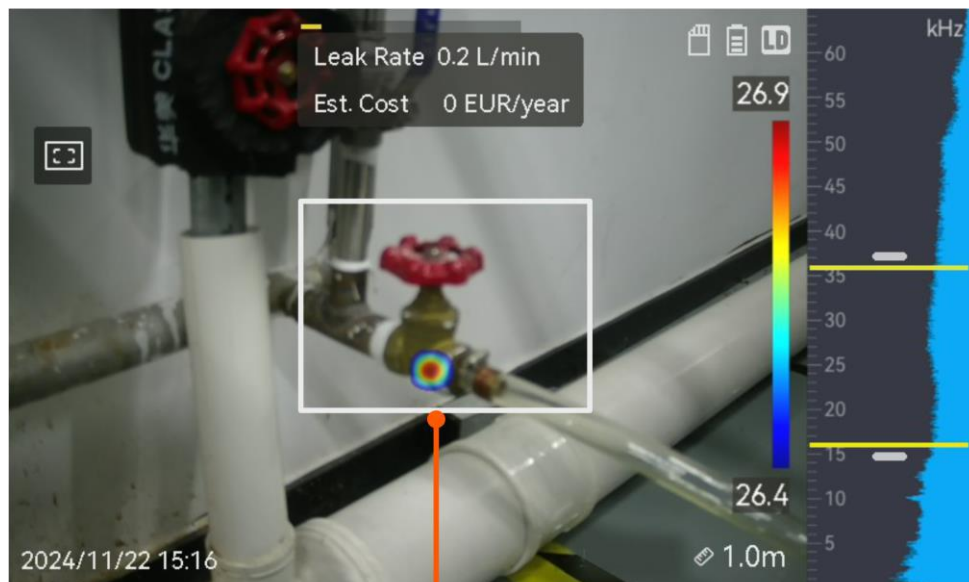
2. Go to **Settings > Display Settings > Sound Intensity**.
3. Enable **Peak**.
4. Press ↶ to save and exit.

5.5.2 Regional Detection Frame

If the target sound source is small and there is sound interference around, enable the regional detection frame and aim the frame to the target. Sound detection only carries out in the framed area.

Tap  once to turn on regional detection frame.

Tap again to switch to / for resizing the regional detection frame.



Regional Detection Frame

Figure 5-3 Regional Detection Frame

5.5.3 Show Multiple Sound Sources

Usually, camera only displays acoustic palettes at the strongest sound source. If you want to see other sound sources in the scene, turn on **Multiple Sources** from **Settings > Acoustic Settings > Multiple Sources**.



In practice, multiple sound source mode is hard to avoid the influence of reflected sound sources. In cases that pipes for inspection are close to ceiling or wall, detected multiple sources are likely several reflections of one leak point. Thus, we are not recommended to use the mode in scenarios with strong reflection.

5.5.4 Ultrasonic to Audible

Normally, human ear can hear sound with its frequency ranges from about 20 to 20,000 Hz. Sound of higher frequency should be converted to audible sound for hearing.

Camera supports **Ultrasonic to Audible** function for the conversion. Connect the camera to Bluetooth headphones for listening to real-time ultrasonic sound sources.



- Users should prepare a pair of Bluetooth headphones.
 - After enabling **Ultrasonic to Audible**, ultrasonic sound in recorded videos is also converted.
 - Converted sound source can not be played with the camera speaker.
 - **Ultrasonic to Audible** function is paused when other audio files (voice note and audio in video clips) are played.
-

Steps




1. Connect your camera to a pair of Bluetooth headsets. See *8.3 Pair Bluetooth*.
2. Enable **Ultrasonic to Audible** function.
 - 1) In live view interface, tap  or press  to show the menu.
 - 2) Go to **Settings > Acoustic Settings > Ultrasonic to Audible**.
 - 3) Enable the function and an ear icon shows in the live image.
3. Listen to the real-time audio and adjust volume.
 - 1) Tap on the  on the screen.
 - 2) Slide the volume bar for adjustment.



Figure 5-4 Ultrasonic to Audible and Volume Adjustment




6 Display Settings

6.1 Set Acoustic Palettes

Acoustic palettes are the shaped colors overlaying on visual image indicating the location and strength of detected sound sources. Palette color, opacity and intensity range of palettes are adjustable.

6.1.1 Set Palette Color

Steps

1. Press  in live view interface to show the menu.
2. Select  from the main menu, go to **Acoustic Settings > Palettes**, and select a desired color combination.
3. Press  to save and exit.




Result

Acoustic palette overlaid above the sound source and palette bar changes to the selected palette.

6.1.2 Set Palette Opacity

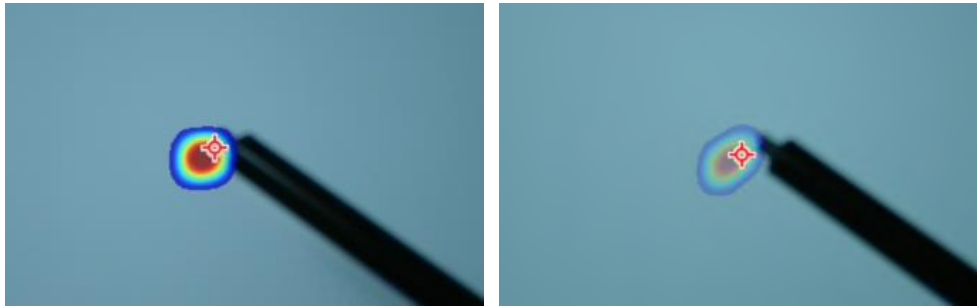
You can view the acoustic palette and the visual images at the same time if the opacity is properly set.

Steps

1. In live view interface, tap  or press  to show the menu.
2. Go to **Settings > Acoustic Settings > Palettes Opacity**, and select a desired level.
3. Press  to save and exit.



The opacity level ranges from 0% to 100%. The lower the value is, the more transparent the acoustic palette is.










Level: 75% vs Level: 25%

6.1.3 Set Intensity Range for Palettes

Colors in palettes stand for different sound intensity values. Usually, camera automatically calculates intensity range for palettes. You can also manually set a fixed range if the auto palette display is not satisfactory.

- **Auto (default):** Camera calculates the upper limit, lower limit, and the intensity delta automatically.
- **Manual:** Camera calculates the upper limit and lower limit of intensity according to the set intensity delta and actual intensity of target sound source.

Steps

1. In live view interface, tap  or press  to show the menu.
2. Go to **Settings > Acoustic Settings > Intensity Range**, and press  to switch to **Manual**.
3. Select **Intensity Delta** and press .
4. Press/hold  and  to adjust values.
5. Press  to save and exit.

6.2 Adjust Digital Zoom



The camera supports 1× to 16× digital zoom.

- In live view interface, hold $\triangle\oplus$ or $\nabla\ominus$ to zoom in or zoom out by 1× continuously.
- In live view interface, press $\triangle\oplus$ or $\nabla\ominus$ to zoom in or zoom out by 0.1× precisely.

6.3 Set Grayscale of Visual Image

The colored live view image turns to black and white if grayscale image is enabled. The black and white image makes colored acoustic palettes more prominent for observation.

Steps

1. In live view interface, tap  or press $\odot\mathbb{K}$ to show the menu.
2. Go to **Settings > Display Settings**.
3. Enable **Grayscale Image**.
4. Press  to save and exit.

6.4 Set Video Standard

Video standard refers to the standard used in the visual camera. Set it according to the mains frequency in your country/region. PAL and NTSC are selectable.




Striped image may occur if wrong video standard is in use.

Go to **Settings > Device Settings > Video Standard** to switch standards. It takes effect after camera restart.

6.5 Set Screen Brightness

Steps

1. In live view interface, tap  or press $\odot\mathbb{K}$ to show the menu.

2. Select  from the main menu, go to **Device Settings > Screen Brightness**.
 - Auto: The camera adjusts screen brightness automatically according to the ambient brightness.
 - Manually: Drag the brightness adjustment slider to the left or right to manually adjust screen brightness.



You can also manually adjust brightness from swipe-down menu.








Figure 6-1 Brightness Adjustment Slider

6.6 On-Screen Display Info.

On-Screen Display (OSD) information informs you the status, time and date, and other information of the camera in live view interface.

Steps

1. In live view interface, tap  or press  to show the menu.
2. Go to **Settings > Display Settings**.
3. Tap  or press  to select the on-screen information.
4. Press  to save and exit.

7 Snapshot and Video

Take snapshots or record videos of inspections or suspected targets for further analysis or other purposes. Snapshots and videos saved in the camera can be exported to PC via USB cable.



- Camera does not support capturing or recording when the menu is shown.
 - When the camera is connected to your PC, it does not support capturing or recording.
 - Go to **Settings > Device Settings > Device Initialization** to initialize the memory card if needed.
-

7.1 Capture Snapshot


Operate the camera to capture live images and save the snapshots in local albums.


Before You Start

Make sure that there is a working memory card mounted in your camera. See *1.3 Appearance* to locate the memory card slot of your camera.

Steps

1. Set a capture mode and pull **Trigger** in live view interface to capture snapshots. There are 3 modes available. Each mode requires different operations.
 - 1) Go to **Settings > Capture Settings > Capture Mode**.
 - 2) Select a mode.
 - **Capture One Image**: Pull **Trigger** once to capture one snapshot.
 - **Scheduled Capture**: Set the capture **Interval** and **Number**. Pull **Trigger** in live view, and the camera captures snapshots according

to the set interval and amount. Pull **Trigger** again or press  to stop capturing.

3) Press  to return to the live view interface.

4) Aim the lens to your target and pull **Trigger** to capture snapshots.

2. **Optional:** After capturing, you can tap the thumbnail of the captured snapshot to view and edit the image.

What to do next

- Go to albums to view and manage files and album folders. See *7.4.1 Manage Albums* and *7.4.2 Manage Files* for operation instructions.
- To edit saved images, see *7.4.3 Edit Files* for operation instructions.
- You can connect your camera to PC to export local files for further use. See *7.5 Export Files*.



7.2 Record Video

You can record videos of the target. The recorded video and audio are saved in the memory card.

Steps

1. In live view interface, hold the trigger to start recording. The recording status icon and time icon appear.
2. When you finish, pull the trigger again to stop recording. The recorded video will be saved automatically and exit.



You can also press  or  to stop recording.

3. Refer to *7.5 Export Files* to export videos.



The video format is MP4 format. You can play videos on the camera or export to the compatible players to play.

7.3 File Naming Rule

Naming rule of captured pictures and videos is allowed to change. Go to **Settings > Capture Settings** to set **Filename Header** and **File Naming**.




Table 7-1 File Naming Rule

| Element | Description |
|-----------------|---|
| Filename Header | File name starts with the set header. |
| File Naming | Time Stamp or Numbering are selectable. Time stamp includes year, month, day, hour, minute, and second. |


7.4 View and Manage Local Files

Camera captured snapshots and videos are saved in local albums. You can create, delete, rename and set an album as the default saving album. For files, operations, such as browsing, moving and deleting, are available.









Steps

1. Enter album.
 - In live view, press  to enter albums.
 - In live view, press  to call the main menu, and select  to enter albums.
2. To create, rename, delete and set an album as the default saving album, see *7.4.1 Manage Albums* for instructions.
3. For file operations, such as, moving or deleting a file, see *7.4.2 Manage Files* for instructions.
4. To modify an image, for example, editing the text or voice notes saved with the images, see *7.4.3 Edit Files* for instructions.

7.4.1 Manage Albums

You can create several albums to manage captured snapshots and video files on your camera. Newly captured snapshots and videos are saved in the **Default Saving Album** .

Steps

1. Enter albums.
 - In live view, press  to enter albums.
 - In live view, press  to call the main menu, and select  to enter albums.
2. Create an album.
 - 1) Tap  in upper right corner to add an album.
 - 2) Edit the album name.
 - 3) Press  to save the album.
3. Rename, delete or set an album as the default saving album.
 - 1) Select an album and press .
 - 2) Tap  in upper right corner of the screen.
 - 3) Select Set as Default Saving Album, Rename or Delete as required.
 - 4) The album icon turns to  when it is set as the default saving album.

7.4.2 Manage Files

Steps















1. Enter albums.
 - In live view, press  to enter albums.
 - In live view, press  to call the main menu, and select  to enter albums.
2. Select an album and press .
3. Browse the image and video files.
 - 1) Select a file and press .
 - 2) Press  and  to browse the previous or the next file.
 - 3) Press  to call the operation menu to check more available operations. File formats and their supported operations are shown below.


Table 7-2 File Formats and Operations

| File Type | Format | Descriptions |
|-----------|--|---|
| Images | File Name.pd.jpeg File Name.ld.jpeg | Editing text and voice notes, moving files, checking basic information, and deleting files are supported on camera. |

| File Type | Format | Descriptions |
|-----------|--------------------------------------|---|
| Videos | File Name.pd.mp4 File Name.ld.mp4 | Playing, moving and deleting video files are supported on camera. |

4. Moving or deleting several files.

- 1) In an album, tap  in the upper right corner of the screen.
- 2) Press  and  to select a file and press . If you want to select all files, tap  in the upper right corner. If you want to cancel all selection, tap .

A selected file displays with a  in its upper right corner.

3) Tap Delete or Move.

- If you tap delete, files are deleted after confirmation.
- If you tap move, select a target album to start moving.

7.4.3

Edit Files

Editing the text, voice or tag notes saved with the images.

Steps
















1. Enter albums.
 - In live view, press  to enter albums.
 - In live view, press  to call the main menu, and select  to enter albums.
2. Select an album and press .
3. Select a file and press  to call the editing menu.
4. Select an option and complete corresponding operations.

Table 7-3 Editing and Managing Images

| Icon | Description |
|---|---|
|  | Editing text note. Add a new text note or change the existed note, and press  to save the settings. |
|  | Editing voice note. You can add a new voice note, play or delete an existed voice note. If the file already has a voice note, tap to play or delete the note. If the file has no voice note attached, press  or tap  to record one. |

| Icon | Description |
|---|---|
|  | Editing tag notes. Tag notes are predefined texts that can be added to the images quickly. Tag note template should be imported to the camera before you can use it. See <i>7.4.4 Import and Manage Tag Note Templates</i> . <ol style="list-style-type: none"> 1. Select Tag Note. 2. Select a tag name. 3. Select tag an option or multiple options, and press OK. 4. Press < and > to switch to the previous or next tag for configuration. |
|  | Move the file to other albums. Select a target album and press OK to confirm the moving. |
|  | Show basic information of the file, for example, the saving time and resolution. |
|  | Delete file. |
|  | Play video. |


7.4.4 Import and Manage Tag Note Templates

Tag note templates contains the predefined tag name and options. With the template imported and activated, users can quick add tags to captured snapshots.

Tag note templates are generated on the client software HIKMICRO Analyzer Acoustic. Copy the templates of json format to the storage of your camera, then you can use and manage the templates.

1. Generate tag note templates on HIKMICRO Analyzer Acoustic.



- Download HIKMICRO Analyzer Acoustic client software from our website. See *7.6 Analyze Snapshot via HIKMICRO Analyzer Acoustic* for more information.
- Click on  at the upper right corner of the software window to get operation guide.
- Software generated templates are saved in the path of PC: Public\HIKMICRO Analyzer Acoustic\TextRemarkTemplate.

2. Connect your camera to PC by the supplied cable. Copy and paste the template files to the TextNote folder of the camera storage.



If more than one templates are imported, the first template is the active one by default. Up to 10 templates can be imported.

3. Go to **Settings > Capture Settings > Tag Note Template** to manage templates.
 - 1) Select a template.
 - 2) Tap on **...** at the upper right corner of screen.
 - 3) Set the template as the default template or delete the template.

7.5 Export Files

Connecting the camera to your PC with supplied cable, you can export the recorded videos and captured snapshots.



- Plug the Type-C male connector of USB cable to the camera and the other type-A connector to PC.
 - You can export the files using USB cable while the camera is turned off.
 - You can export the files by inserting the memory card to your PC which has a card slot.
-

Steps

1. Open the cover of cable interface.
 2. Connect the camera to your PC with cable and open the detected disk.
 3. Select and copy the videos or snapshots to PC to view the files.
 4. Disconnect the camera from your PC.
-




You can play the recorded videos using the default players.

7.6 Analyze Snapshot via HIKMICRO Analyzer Acoustic

Captured snapshots can be imported to HIKMICRO Analyzer Acoustic PC client for analysis and report generating.

Visit our website <http://www.hikmicrotech.com>, or contact us to get the software.

Click on  at the upper right corner of the software window to get operation guide.

8 Connections

8.1 Connect Camera to Wi-Fi

Steps






1. Enter Wi-Fi setting interface. Choose from the following ways.
 - Tap  from the swipe-down menu.
 - Go to **Settings > Connections > WLAN**.
2. Tap  to enable Wi-Fi, and the searched Wi-Fi will be listed.



Figure 8-1 Wi-Fi List

3. Set and Join a Wi-Fi.

Using Wi-Fi password

1. Tap an available Wi-Fi, and a soft keyboard is displayed.
2. Set the Wi-Fi password with the soft keyboard.
3. Tap  to save.  shows in live view interface and  shows on the right side of the connected Wi-Fi when the connection is completed.
4. Enable the Wi-Fi function of other equipment and search the Wi-Fi that the camera is in to join.



DO NOT tap space, or the password may be incorrect.

Using Wi-Fi QR

1. Scan the QR code using HIKMICRO Viewer to

code

quickly join the Wi-Fi and connect the camera to the APP. For more information about the APP, see *8.4 Connect to HIKMICRO Viewer APP*.

8.2 Set Camera Hotspot

When the camera's hotspot is on, other equipment with Wi-Fi function can join the camera for data transmission.

Steps




1. Enter hotspot configuration interface. Choose from the following ways.
 - Tap  from swipe-down menu.
 - Go to **Settings > Connections > Hotspot**.
2. Tap  to enable hotspot function.



Figure 8-2 Hotspot

3. Set and join the hotspot.

Using hotspot password

1. Tap **Set Hotspot**. A soft keyboard is displayed.
2. Set the password for the hotspot with the soft keyboard.
3. Tap  to save.
4. Enable the Wi-Fi function of other equipment and search the camera hotspot to join.

Using hotspot QR code

1. Scan the QR code using HIKMICRO Viewer to quickly join the hotspot and connect the camera to the APP. For more information about the APP, see *8.4 Connect to HIKMICRO Viewer APP*.






- When setting password, do not tap **space**, or the password may be incorrect.
 - The password should be at least 8 digits, consisting of numbers and characters.
-

8.3 Pair Bluetooth Devices

Pair your camera with an external Bluetooth player (speaker or headsets) to play the recorded audios or converted live ultrasonic sound sources.

Steps

1. Enter Bluetooth configuration page. Choose from the following ways.
 - Tap  from swipe-down menu.
 - Select  from the main menu. Go to **Settings > Connections > Bluetooth**.
2. Tap on  to enable the Bluetooth. The camera searches and displays available nearby Bluetooth devices.



Make sure the external Bluetooth device is in discoverable mode.

3. Select an external Bluetooth device to start automatic pairing and connecting.



The Bluetooth function is for audio play only. If you want to exporting local files, see *7.5 Export Files* for instructions.

8.4 Connect to HIKMICRO Viewer APP

HIKMICRO Viewer is a mobile APP working with the camera. With the APP, you can:

- View camera live image.
- Visit camera local album, download snapshots and videos.
- Upgrade camera firmware.

Follow the steps to connect the camera to the APP.

Before You Start

Download and install HIKMICRO Viewer to your phone. Search the APP name in your APP store, or scan the following QR code.



Steps

1. Add your camera and your phone to the same local network.
 - Use camera Wi-Fi, see *8.1 Connect Camera to Wi-Fi*.
 - Use camera Hotspot, see *8.2 Set Camera Hotspot*.
2. (Ignore this step if camera is added via Wi-Fi/hotspot QR code) Connect your camera to the APP:
 - 1) Launch HIKMICRO Viewer.
 - 2) Tap on + > **Add Device** to add the device. “Connected” is displayed in home screen of the APP.

What to do next

Tap on **Live View**, **On-Device File**, or **Device Upgrade** to perform other functions.

9 Cast Screen

The device supports casting screen to PC by software clients compliant with UVC protocol.

Before You Start


Download and install a software client compliant with UVC protocol on your PC.

Steps

1. Launch the software client on your PC.
2. Use a USB cable to connect your device with the PC.



Make sure that your camera is on and with sufficient power.

3. In pop-up window of your device, select **USB Cast Screen**.  will be displayed in the device status bar.
4. Click “connect” or “refresh” in the software client.

Results

The live image of your device is displayed in the PC.

10 Maintenance

10.1 View Camera Information

Go to **Settings > Device Settings > Device Information** to view the camera information.

10.2 Set Language

Go to **Settings > Device Settings > Language** to set system language.

10.3 Set Time and Date

Steps

1. Press **OK** to show the menu in live view interface.
2. Go to **Settings > Device Settings > Time and Date**.
3. Set the date and time.
4. Press **↩** to save and exit.



Go to **Settings > Display Settings** to enable or disable time and date on-screen display.

10.4 Upgrade Camera

Upgrade the camera via an upgrade file, or via HIKMICRO Viewer APP.

10.4.1 Upgrade with HIKMICRO Viewer APP

Connect your camera to HIKMICRO Viewer APP and tap on **Device Upgrade** to check camera firmware version and proceed online upgrading. See *8.4 Connect to HIKMICRO Viewer APP* for more details.

10.4.2 Upgrade with an Upgrade File

Before You Start

- Please download the upgrade file from the official website <http://www.hikmicrotech.com> or contact the customer service and technical support to get the upgrade file first.
- Make sure that the camera battery is fully charged.
- Make sure that Auto Power-off function is turned-off to avoid accidental suspension during upgrading.
- Make sure that a memory card has been installed to camera.

Steps

1. Connect the camera to your PC with a Type-C to type A cable and open the detected disk.
2. Copy the upgrade file and paste it to the root directory of the camera.
3. Disconnect the camera from your PC.
4. Reboot the camera and then it will upgrade automatically. The upgrading process will be displayed in the main interface.



After upgrading, the camera reboots automatically. You can view the current version in **Settings > Device Settings > Device Information**.

10.5 Restore Camera

You can default the camera to the factory settings.



This function should be used with caution.

Steps

1. Press **OK** to show the menu in live view interface.

2. Go to **Settings > Device Settings > Device Initialization**.
3. Select **Restore Device**. A prompt appears.
 - **OK**: Tap **OK** to initialize the device.
 - **Cancel**: Tap **Cancel** to exit and return to the previous menu.

10.6 Record Sound Source for Trouble Shooting

Record sound source function is to save original audio files for trouble shooting when microphone error occurs.

Steps

1. Go to **Settings > Capture Settings > Record Sound Source** to enable the function.
2. Return to live view, aim the microphone array to a sound source and hold the trigger to start video recording.
3. Pull the trigger to stop recording. Or the recording stops when it reaches the maximum length (20 seconds).
4. Export the audio file and send the file to your dealer or our technical support for trouble shooting.



- The audio files are not available in the local album. Connect your camera to a PC, then check and export the files, see *7.5 Export Files* for instructions.
 - The audio files are saved in DCIM folder. The file name is the same as the video file, and the format is *.sonic.
-

10.7 Save Log

Camera supports saving operation logs for trouble shooting. The logs are saved in log folder under the root directory of the camera storage/memory card. Connect the camera to a PC to export the logs.

Steps

1. Go to **Settings > Device Settings > Save Log** to enable the function.

2. Camera starts saving operation logs. It stops when you turn off the function or when the camera restarts or powers off.



You need to enable the function again if you need the camera to save logs after a restart.

3. Visit the device storage/memory card and copy the log files (*.tar) to your PC and send the file to our technical support. See *7.5 Export Files* for instructions.

11 More Information

Scan the following QR code to get device common FAQ.



Legal Information


© Hangzhou Microimage Software Co., Ltd. All rights reserved.

About this Manual

The Manual includes instructions for using and managing the Product. Pictures, charts, images and all other information hereinafter are for description and explanation only. The information contained in the Manual is subject to change, without notice, due to firmware updates or other reasons. Please find the latest version of this Manual at the HIKMICRO website (<http://www.hikmicrotech.com>).

Please use this Manual with the guidance and assistance of professionals trained in supporting the Product.

Trademarks

 **HIKMICRO** and other HIKMICRO's trademarks and logos are the properties of HIKMICRO in various jurisdictions.

HDMI[®]: The terms HDMI and HDMI High-Definition Multimedia Interface, and the HDMI Logo are trademarks or registered trademarks of HDMI Licensing Administrator, Inc. in the United States and other countries.

Other trademarks and logos mentioned are the properties of their respective owners.

Disclaimer

TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW, THIS MANUAL AND THE PRODUCT DESCRIBED, WITH ITS HARDWARE, SOFTWARE AND FIRMWARE, ARE PROVIDED "AS IS" AND "WITH ALL FAULTS AND ERRORS". HIKMICRO MAKES NO WARRANTIES, EXPRESS OR IMPLIED, INCLUDING WITHOUT LIMITATION, MERCHANTABILITY, SATISFACTORY QUALITY, OR FITNESS FOR A PARTICULAR PURPOSE.

THE USE OF THE PRODUCT BY YOU IS AT YOUR OWN RISK. IN NO EVENT WILL HIKMICRO BE LIABLE TO YOU FOR ANY SPECIAL, CONSEQUENTIAL, INCIDENTAL, OR INDIRECT DAMAGES, INCLUDING, AMONG OTHERS, DAMAGES FOR LOSS OF BUSINESS PROFITS, BUSINESS INTERRUPTION, OR LOSS OF DATA, CORRUPTION OF SYSTEMS, OR LOSS OF DOCUMENTATION, WHETHER BASED ON BREACH OF CONTRACT, TORT (INCLUDING NEGLIGENCE), PRODUCT LIABILITY, OR OTHERWISE, IN CONNECTION WITH THE USE OF THE PRODUCT, EVEN IF HIKMICRO HAS BEEN ADVISED OF THE POSSIBILITY OF SUCH DAMAGES OR LOSS.

YOU ACKNOWLEDGE THAT THE NATURE OF THE INTERNET PROVIDES FOR INHERENT SECURITY RISKS, AND HIKMICRO SHALL NOT TAKE ANY RESPONSIBILITIES FOR ABNORMAL OPERATION, PRIVACY LEAKAGE OR OTHER DAMAGES RESULTING FROM CYBER-ATTACK, HACKER ATTACK, VIRUS INFECTION, OR OTHER INTERNET SECURITY RISKS; HOWEVER, HIKMICRO WILL PROVIDE TIMELY TECHNICAL SUPPORT IF REQUIRED.

YOU AGREE TO USE THIS PRODUCT IN COMPLIANCE WITH ALL APPLICABLE LAWS, AND YOU ARE SOLELY RESPONSIBLE FOR ENSURING THAT YOUR USE CONFORMS TO THE APPLICABLE LAW. ESPECIALLY, YOU ARE RESPONSIBLE, FOR USING THIS PRODUCT IN A MANNER THAT DOES NOT INFRINGE ON THE RIGHTS OF THIRD PARTIES, INCLUDING WITHOUT LIMITATION, RIGHTS OF PUBLICITY, INTELLECTUAL PROPERTY RIGHTS, OR DATA PROTECTION AND OTHER PRIVACY RIGHTS. YOU SHALL NOT USE THIS PRODUCT FOR ANY PROHIBITED END-USES, INCLUDING THE DEVELOPMENT OR PRODUCTION OF WEAPONS OF MASS DESTRUCTION, THE DEVELOPMENT OR PRODUCTION OF CHEMICAL OR BIOLOGICAL WEAPONS, ANY ACTIVITIES IN THE CONTEXT RELATED TO ANY NUCLEAR EXPLOSIVE OR UNSAFE NUCLEAR FUEL-CYCLE, OR IN SUPPORT OF HUMAN RIGHTS ABUSES.

IN THE EVENT OF ANY CONFLICTS BETWEEN THIS MANUAL AND THE APPLICABLE LAW, THE LATTER PREVAILS.

Regulatory Information

These clauses apply only to the products bearing the corresponding mark or information.

FCC Compliance Statement

Please take attention that changes or modification not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions:

- (1) this device may not cause harmful interference, and
- (2) this device must accept any interference received, including interference that may cause undesired operation.

This equipment complies with FCC radiation exposure limits set forth for an uncontrolled environment.

For models with 64 microphone array:

Note: This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

EU Conformity Statement



This product and - if applicable - the supplied accessories too are marked with "CE" and comply therefore with the applicable harmonized European standards listed under the Directive 2014/30/EU (EMC), Directive 2014/35/EU (LVD), Directive 2011/65/EU (RoHS).

Hereby, Hangzhou Microimage Software Co., Ltd. declares that this device (refer to the label) is in compliance with Directive 2014/53/EU. The full text of the EU declaration of conformity is available at the following internet address:
<https://www.hikmicrotech.com/en/support/download-center/declaration-of-conformity/>

Restrictions in the 5 GHz band:

According to Article 10 (10) of Directive 2014/53/EU, when operating in the 5150 to 5350 MHz frequency range, this device is restricted to indoor use in: Austria (AT), Belgium (BE), Bulgaria (BG), Croatia (HR), Cyprus (CY), the Czech Republic (CZ), Denmark (DK), Estonia (EE), Finland (FI), France (FR), Germany (DE), Greece (EL), Hungary (HU), Iceland (IS), Ireland (IE), Italy (IT), Latvia (LV), Liechtenstein (LI), Lithuania (LT), Luxembourg (LU), Malta (MT), Netherlands (NL), Northern Ireland (UK(NI)), Norway (NO), Poland (PL), Portugal (PT), Romania (RO), Slovakia (SK), Slovenia (SI), Spain (ES), Sweden (SE), Switzerland (CH), and Turkey (TR).

RF Exposure Information

This device has been tested and meets applicable limits for Radio Frequency (RF) exposure.

Frequency Bands and Power

The frequency bands and modes and transmitting power (radiated and/or conducted) nominal limits applicable to the following radio equipment are as follows:

Wi-Fi: 2.4 GHz (2.4 GHz to 2.4835 GHz): 20 dBm; 5 GHz (5.15 GHz to 5.25 GHz): 23 dBm; 5 GHz (5.25 GHz to 5.35 GHz): 23 dBm; 5 GHz (5.47 GHz to 5.725GHz): 23 dBm; 5 GHz (5.725 GHz to 5.875 GHz): 14 dBm

5G indoors use only.

Use the power adapter provided by a qualified manufacturer. Refer to the product specification for detailed power requirements.

Use the battery provided by a qualified manufacturer. Refer to the product specification for detailed battery requirements.

For models with 64 microphone array:

Warning: This is a class A product. In a domestic environment this product may cause radio interference, in which case, the user may be required to take adequate measures.



Directive 2012/19/EU (WEEE Directive): Products marked with this symbol cannot be disposed of as unsorted municipal waste in the European Union. For proper recycling, return this product to your local supplier upon the purchase of equivalent new equipment, or dispose of it at designated collection points. For more information see: www.recyclethis.info



Regulation (EU) 2023/1542 (Battery Regulation): This product contains a battery and it is in conformity with the Regulation (EU) 2023/1542. The battery cannot be disposed of as unsorted municipal waste in the European Union. See the product documentation for specific battery information. The battery is marked with this symbol, which may include lettering to indicate cadmium (Cd), or lead (Pb). For proper recycling, return the battery to your supplier or to a designated collection point. For more information see: www.recyclethis.info.

Industry Canada ICES-003 Compliance/Conformité Industrie Canada ICES-003

For models with 136 microphone array:

This device meets the CAN ICES-003 (B) / NMB-003 (B) standards requirements.

Cet appareil répond aux exigences des normes CAN ICES-003 (B)/NMB-003 (B).

For models with 64 microphone array:

This device meets the CAN ICES-003 (A) / NMB-003 (A) standards requirements.

Cet appareil répond aux exigences des normes CAN ICES-003 (A)/NMB-003 (A).

This device complies with Industry Canada licence-exempt RSS standard(s). Operation is subject to the following two conditions:

- (1) this device may not cause interference, and
- (2) this device must accept any interference, including interference that may cause undesired operation of the device.

This equipment complies with IC RSS-102 radiation exposure limits set forth for an uncontrolled environment.

For this device, please pay attention to the following notes when the device is operating in 5 GHz:

- (i) The device for operation in the band 5150-5250 MHz is only for indoor use to reduce the potential for harmful interference to co-channel mobile satellite systems;
- (ii) The maximum antenna gain permitted for devices in the bands 5250-5350 MHz and 5470-5725 MHz shall comply with the e.i.r.p. limit; and
- (iii) The maximum antenna gain permitted for devices in the band 5725-5875 MHz shall comply with the e.i.r.p. limits specified for point-to-point and non point-to-point operation as appropriate.

Users should also be advised that high-power radars are allocated as primary users (i.e. priority users) of the bands 5250-5350 MHz and 5650-5850 MHz and that these radars could cause interference and/or damage to LE-LAN devices.

Le présent appareil est conforme aux CNR d'Industrie Canada applicables aux appareils radioexempts de licence. L'exploitation est autorisée aux deux conditions suivantes :

- (1) l'appareil ne doit pas produire de brouillage, et
- (2) l'utilisateur de l'appareil doit accepter tout brouillage radioélectrique subi, même si le brouillage est susceptible d'en compromettre le fonctionnement.

ce matériel est conforme aux limites de dose d'exposition aux rayonnements, CNR-102 énoncée dans un autre environnement.

- (i) Les dispositifs fonctionnant dans la bande 5150-5250 MHz sont réservés uniquement pour une utilisation à l'intérieur afin de réduire les risques de brouillage préjudiciable aux systèmes de satellites mobiles utilisant les mêmes canaux.
- (ii) Le gain d'antenne maximal autorisé pour les appareils dans les

bandes 5250-5350 MHz et 5470-5725 MHz doivent respecter le pire limiter; et

(iii) Le gain d'antenne maximal autorisé pour les appareils dans la bande 5725-5875 MHz doivent respecter le pire limites spécifiées pour le point-à-point et l'exploitation non point à point, le cas échéant.

Les utilisateurs de radars de haute puissance sont désignés utilisateurs principaux (c.-à-d., qu'ils ont la priorité) pour les bandes 5250-5350 MHz et 5650-5850 MHz et que ces radars pourraient causer du brouillage et/ou des dommages aux dispositifs LAN-EL.

KC

For models with 136 microphone array:

B 급 기기: 이 기기는 가정용(B 급) 전자파적합기기로서 주로 가정에서 사용하는 것을 목적으로 하며, 모든 지역에서 사용할 수 있습니다.

For models with 64 microphone array:

A 급 기기: 이 기기는 업무용(A 급) 전자파적합기기로서 판매자 또는 사용자는 이 점을 주의하시기바라며, 가정 외의 지역에서 사용하는 것을 목적으로 합니다.

INFORMATIONEN FÜR PRIVATE HAUSHALTE

1. Getrennte Erfassung von Altgeräten: 1. Getrennte Erfassung von Altgeräten:

Elektro- und Elektronikgeräte, die zu Abfall geworden sind, werden als Altgeräte bezeichnet. Besitzer von Altgeräten haben diese einer vom unsortierten Siedlungsabfall getrennten Erfassung zuzuführen.

Altgeräte gehören insbesondere nicht in den Hausmüll, sondern in spezielle Sammel- und Rückgabesysteme.

2. Batterien und Akkus sowie Lampen:

Besitzer von Altgeräten haben Altbatterien und Altakkumulatoren, die nicht vom Altgerät umschlossen sind, die zerstörungsfrei aus dem Altgerät entnommen werden können, im Regelfall vor der Abgabe an einer Erfassungsstelle vom Altgerät zu trennen. Dies gilt nicht, soweit Altgeräte einer Vorbereitung zur Wiederverwendung unter Beteiligung eines öffentlich-rechtlichen Entsorgungsträgers zugeführt werden.

3. Möglichkeiten der Rückgabe von Altgeräten:

Besitzer von Altgeräten aus privaten Haushalten können diese bei den Sammelstellen der öffentlich-rechtlichen Entsorgungsträger oder bei den von Herstellern oder Vertriebern im Sinne des ElektroG eingerichteten Rücknahmestellen unentgeltlich abgeben.

Rücknahmepflichtig sind Geschäfte mit einer Verkaufsfläche von mindestens 400 m² für Elektro- und Elektronikgeräte sowie diejenigen Lebensmittelgeschäfte mit einer Gesamtverkaufsfläche von mindestens 800 m², die mehrmals pro Jahr oder dauerhaft Elektro- und Elektronikgeräte anbieten und auf dem Markt bereitstellen. Dies gilt auch bei Vertrieb unter Verwendung von Fernkommunikationsmitteln, wenn die Lager- und Versandflächen für Elektro- und Elektronikgeräte mindestens 400 m² betragen oder die gesamten Lager- und Versandflächen mindestens 800 m² betragen. Verreiber haben die Rücknahme grundsätzlich durch geeignete Rückgabemöglichkeiten in zumutbarer Entfernung zum jeweiligen Endnutzer zu gewährleisten. Die Möglichkeit der unentgeltlichen Rückgabe eines Altgerätes besteht bei rücknahmepflichtigen Vertriebern unter anderem dann, wenn ein neues gleichartiges Gerät, das im Wesentlichen die gleichen Funktionen erfüllt, an einen Endnutzer abgegeben wird.

4. Datenschutz-Hinweis:

Altgeräte enthalten häufig sensible personenbezogene Daten. Dies gilt insbesondere für Geräte der Informations- und

Telekommunikationstechnik wie Computer und Smartphones. Bitte beachten Sie in Ihrem eigenen Interesse, dass für die Löschung der Daten auf den zu entsorgenden Altgeräten jeder Endnutzer selbst verantwortlich ist.

5. Bedeutung des Symbols „durchgestrichene Mülltonne“:



Das auf Elektro- und Elektronikgeräten regelmäßig abgebildete

Symbol einer durchgestrichenen Mülltonne weist darauf hin, dass das jeweilige Gerät am Ende seiner Lebensdauer getrennt vom unsortierten Siedlungsabfall zu erfassen ist.



HIKMICRO

See the World in a New Way

Facebook: Hikmicro Industrial
Instagram: hikmicro_industrial
E-mail: support@hikmicrotech.com

LinkedIn: HIKMICRO
YouTube: HIKMICRO Industrial
Website: <https://www.hikmicrotech.com/>

UD42007B